

ELEV 55

NZJC


NON-CERTIFICATED

CHRISTCHURCH HOSPITAL

HELIPORT

CHRISTCHURCH TOWER: 118.4 119.65


CHRISTCHURCH ATIS: 127.2

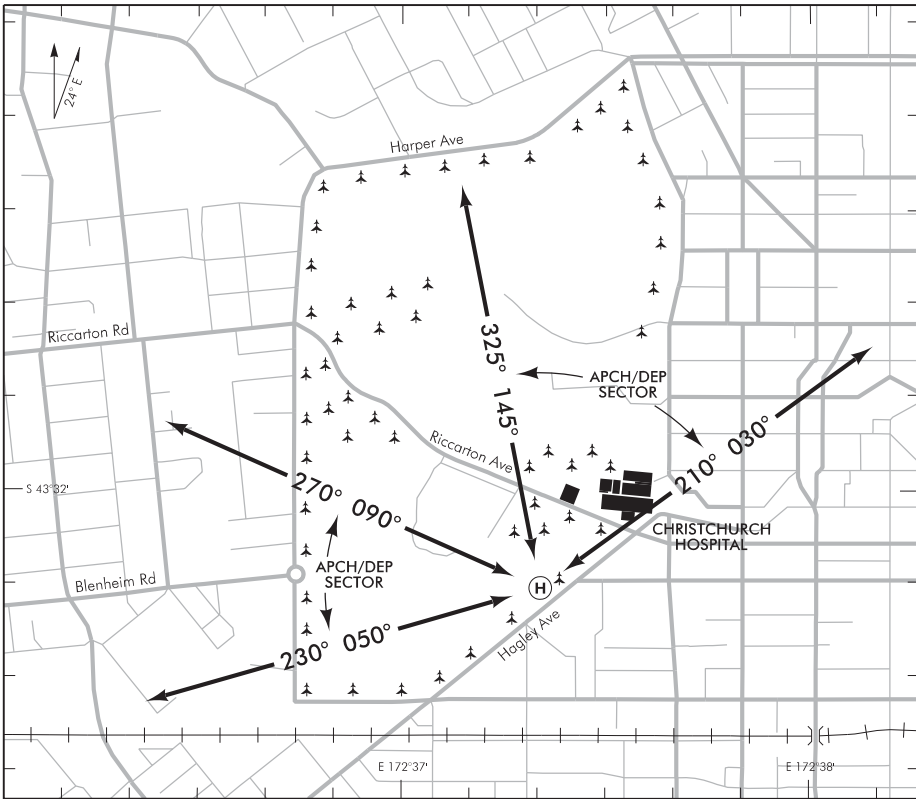

NZJC-B

Changes from 28 JUL 11: TWR FREQ.

Heliport located within Christchurch CTR/C.

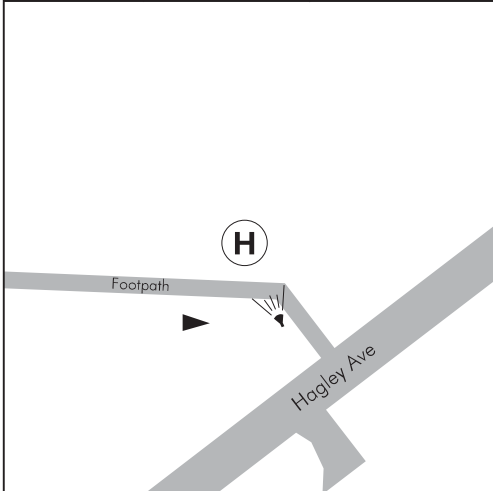

S 43 32 12 E 172 37 20

Effective: 26 MAY 16

CHRISTCHURCH HOSPITAL

© Civil Aviation Authority

HELIPORT

FATO/TLOF

	SIZE	SFC	STRENGTH	MARKINGS
FATO	Diameter 21 m	Gr		Nil
TLOF	Diameter 5 m	Gr		(H)

Maximum helicopter size 13.5 m overall length.

LIGHTING

Non approved.

Inadequate floodlighting. For use in emergency only.

PAL 133.15 Non-standard operation — transmit 4 pulses within 5 seconds.

FACILITIES

Nil

SUPPLEMENTARY

Operator: Canterbury Health Ltd, Private Bag 4710, Christchurch
Tel (03) 364 0640 Fax (03) 364 0099

Available for limited use subject to the prior agreement of the operator.